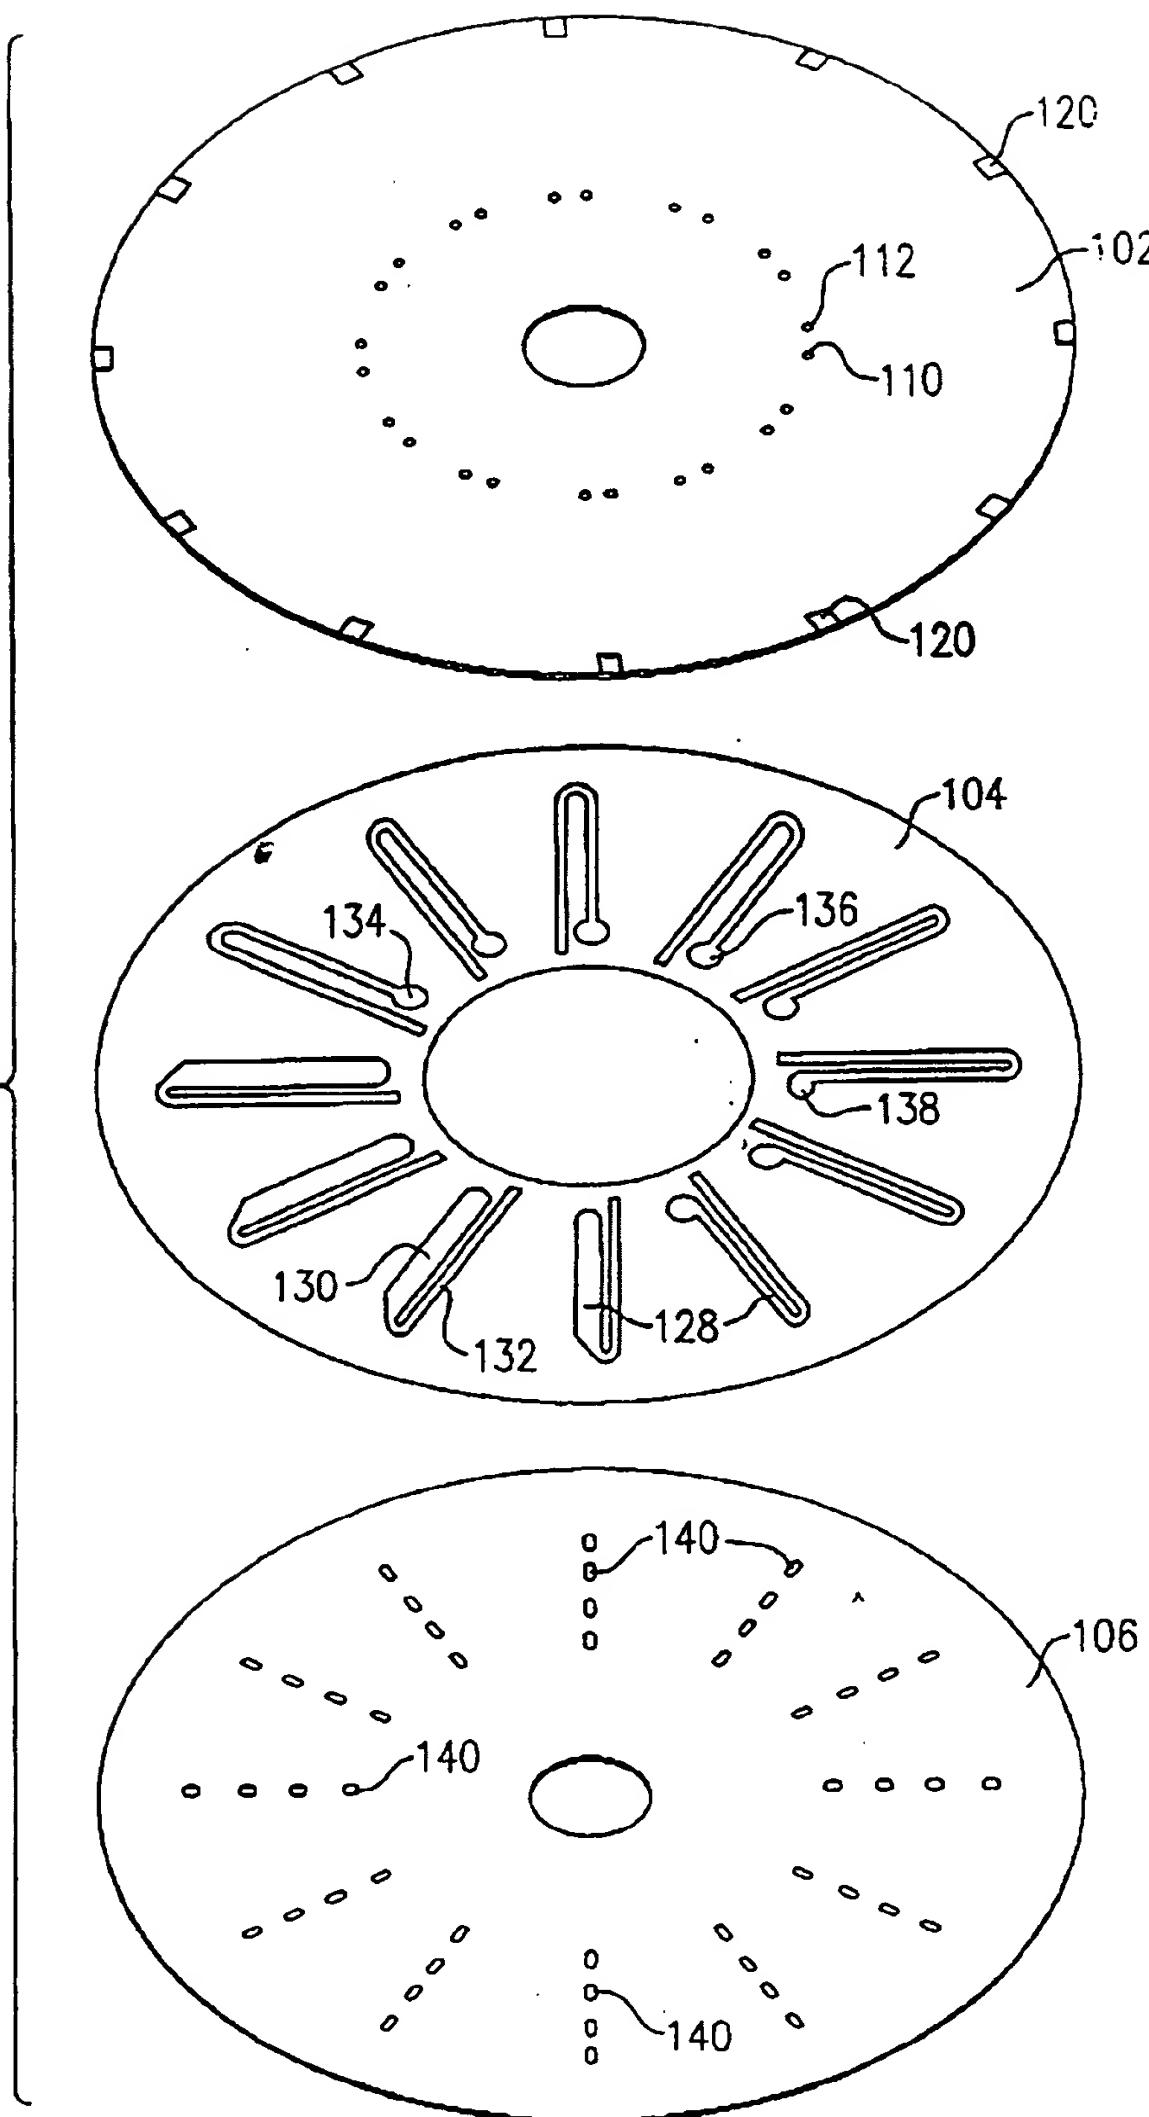


1/18

FIG. 1A



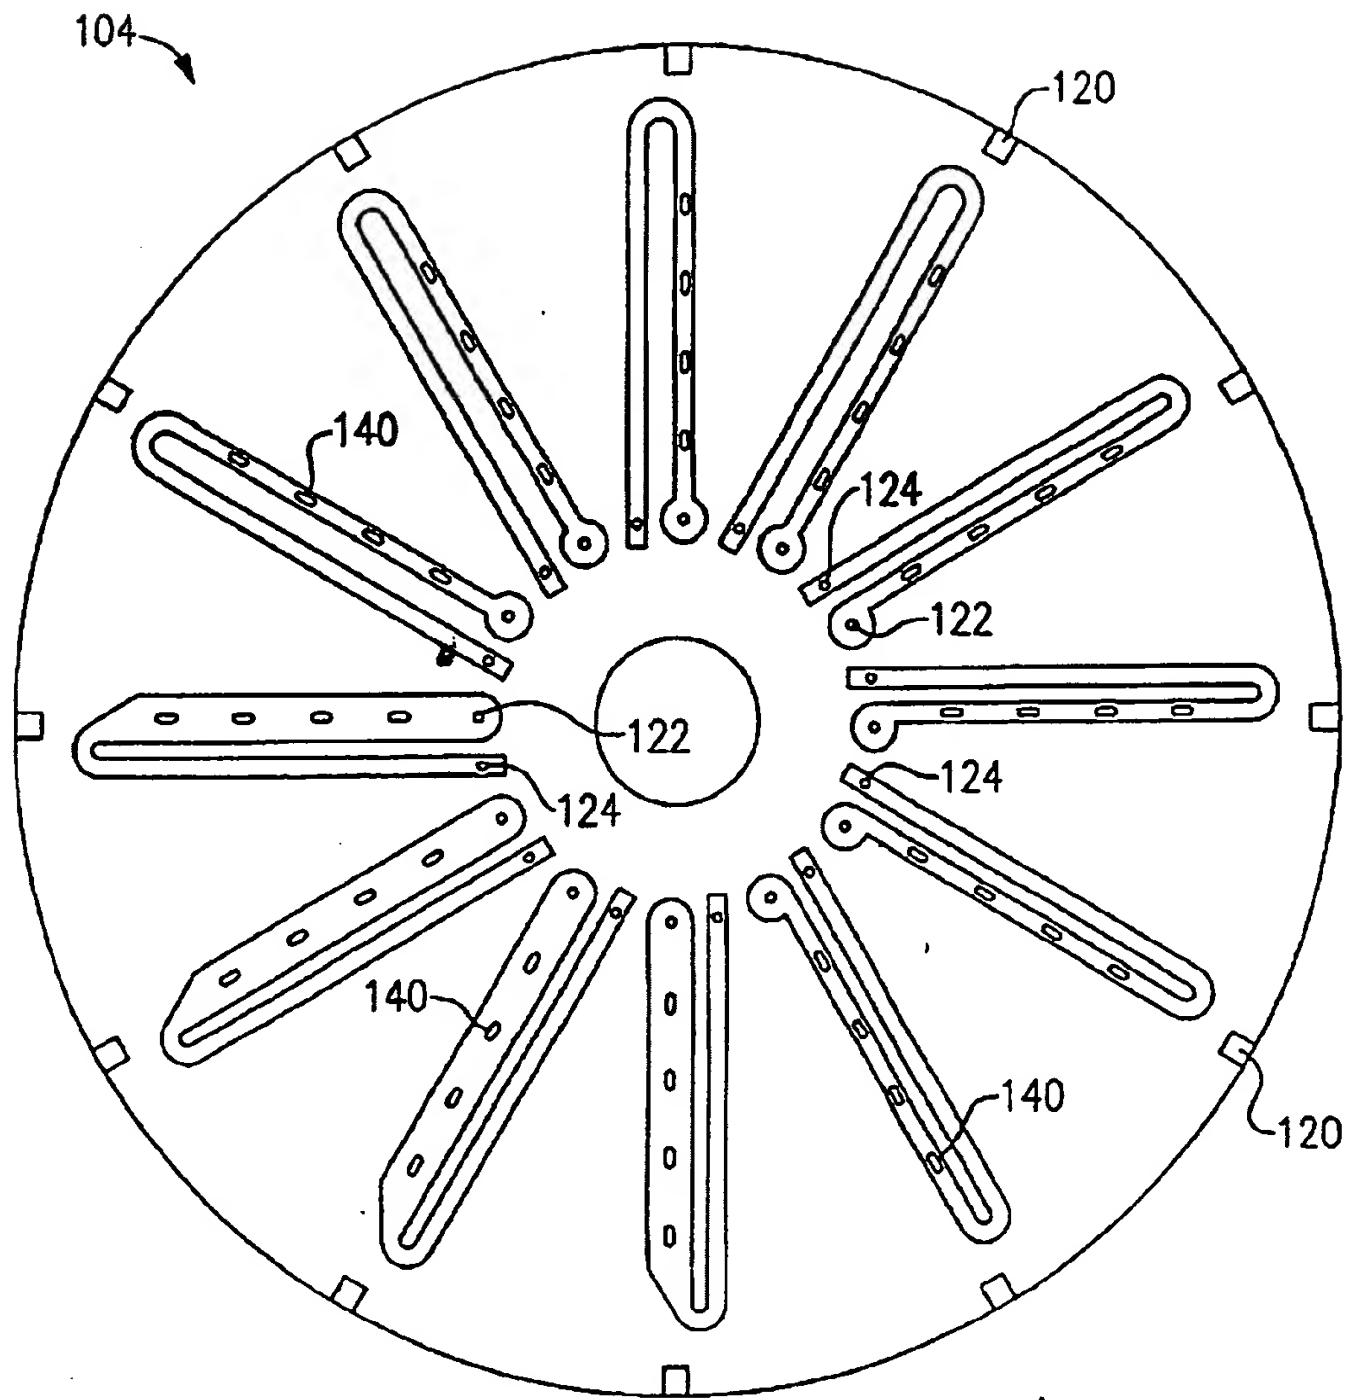
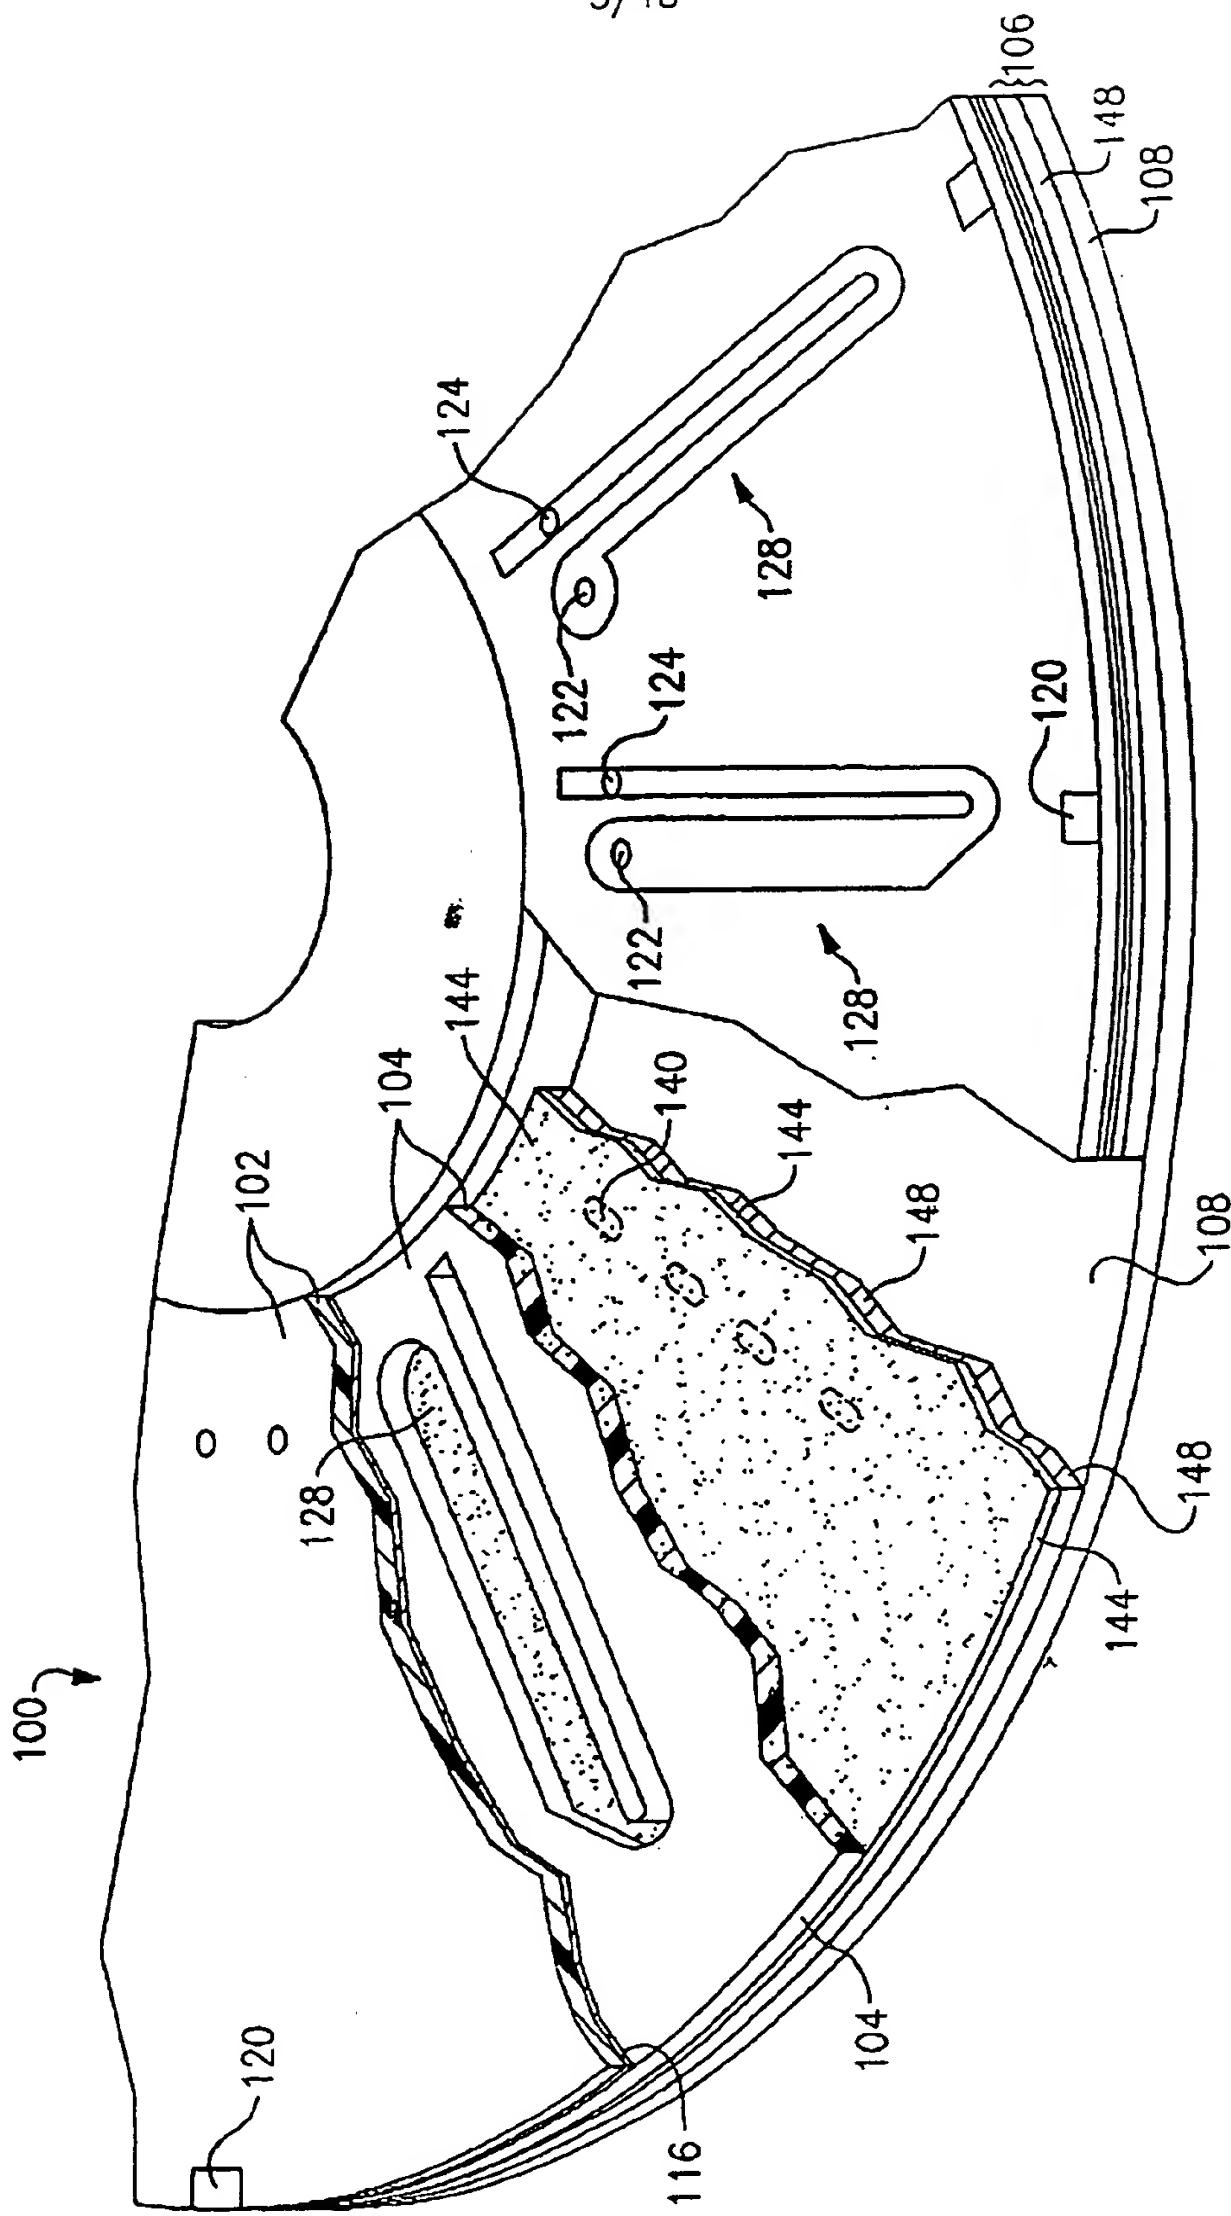


FIG.1B

3/18



**FIG. 1C**

4/18

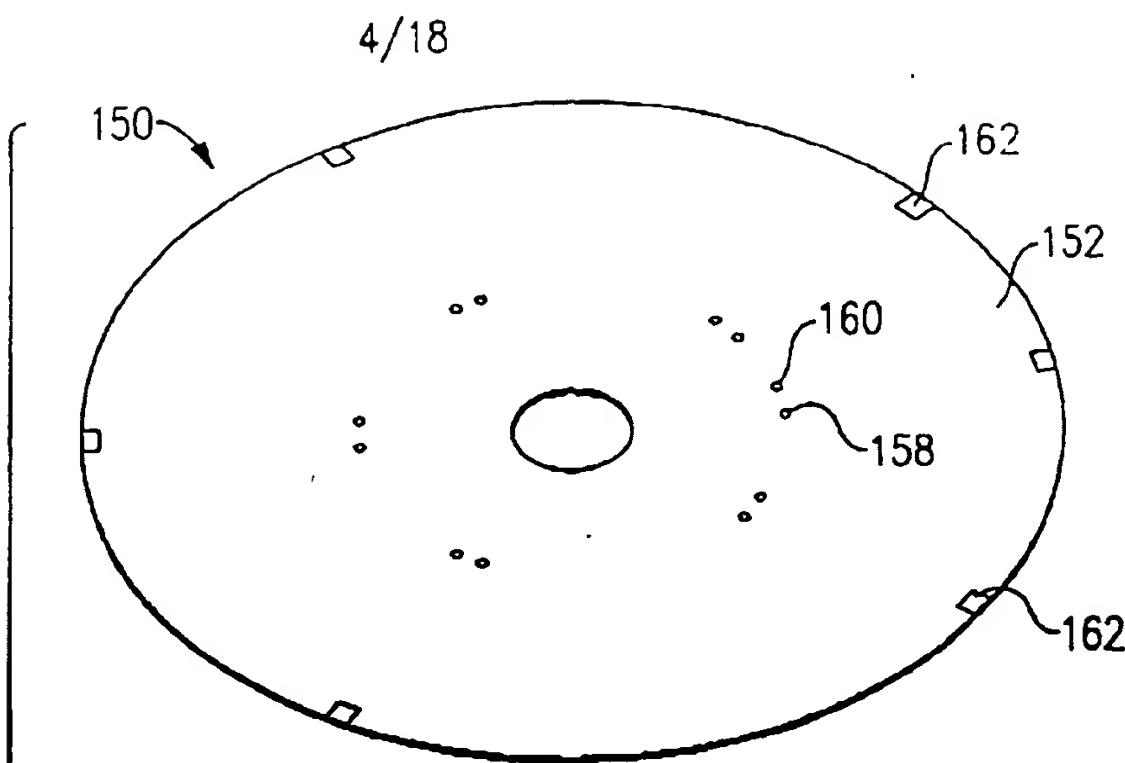
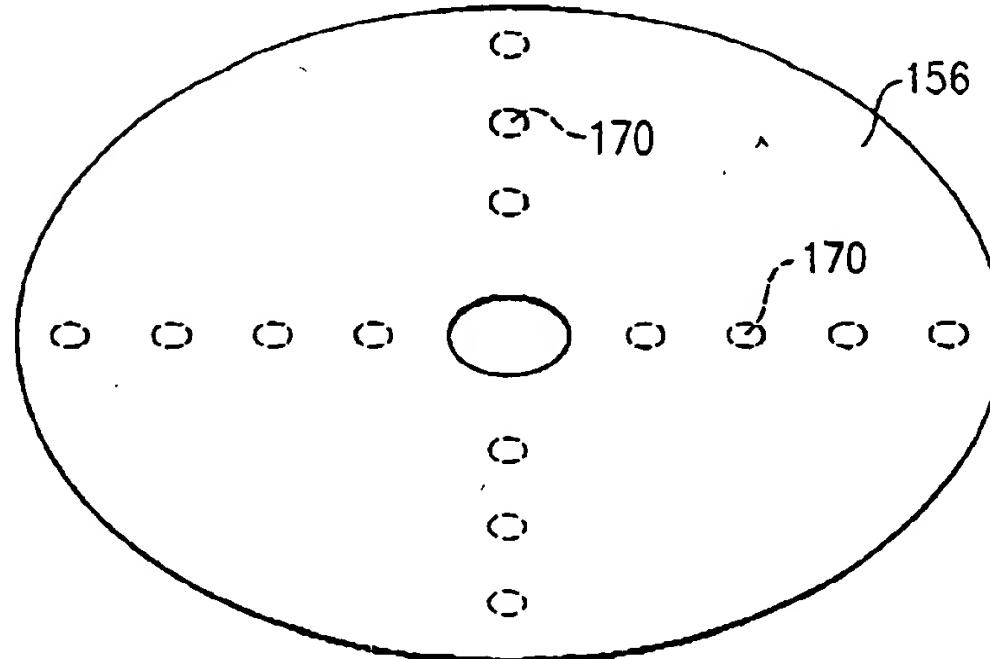
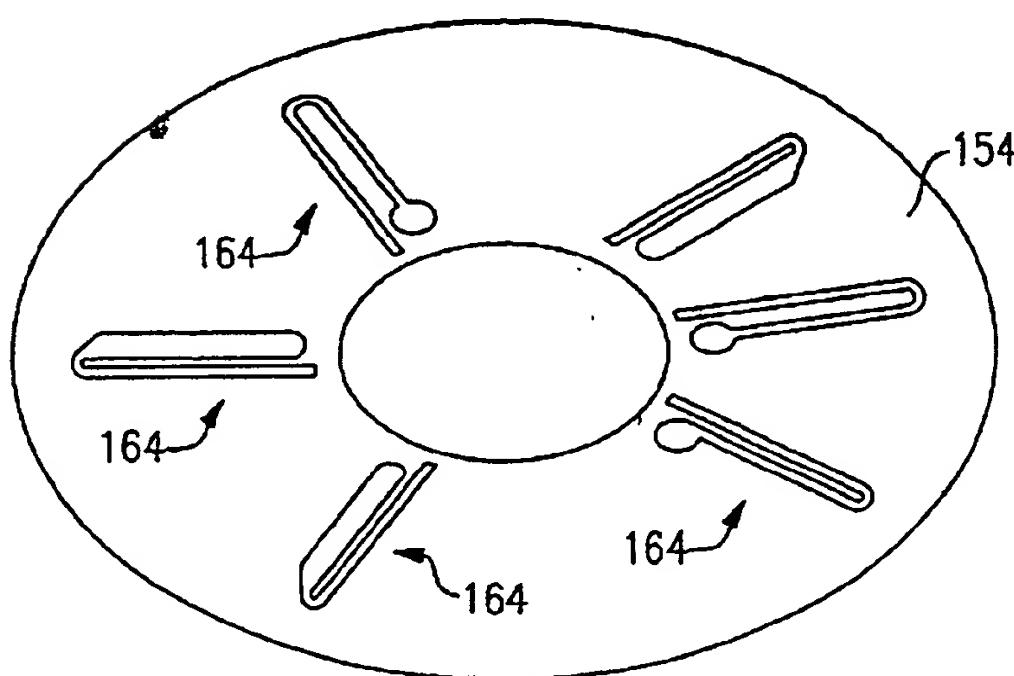


FIG.2A



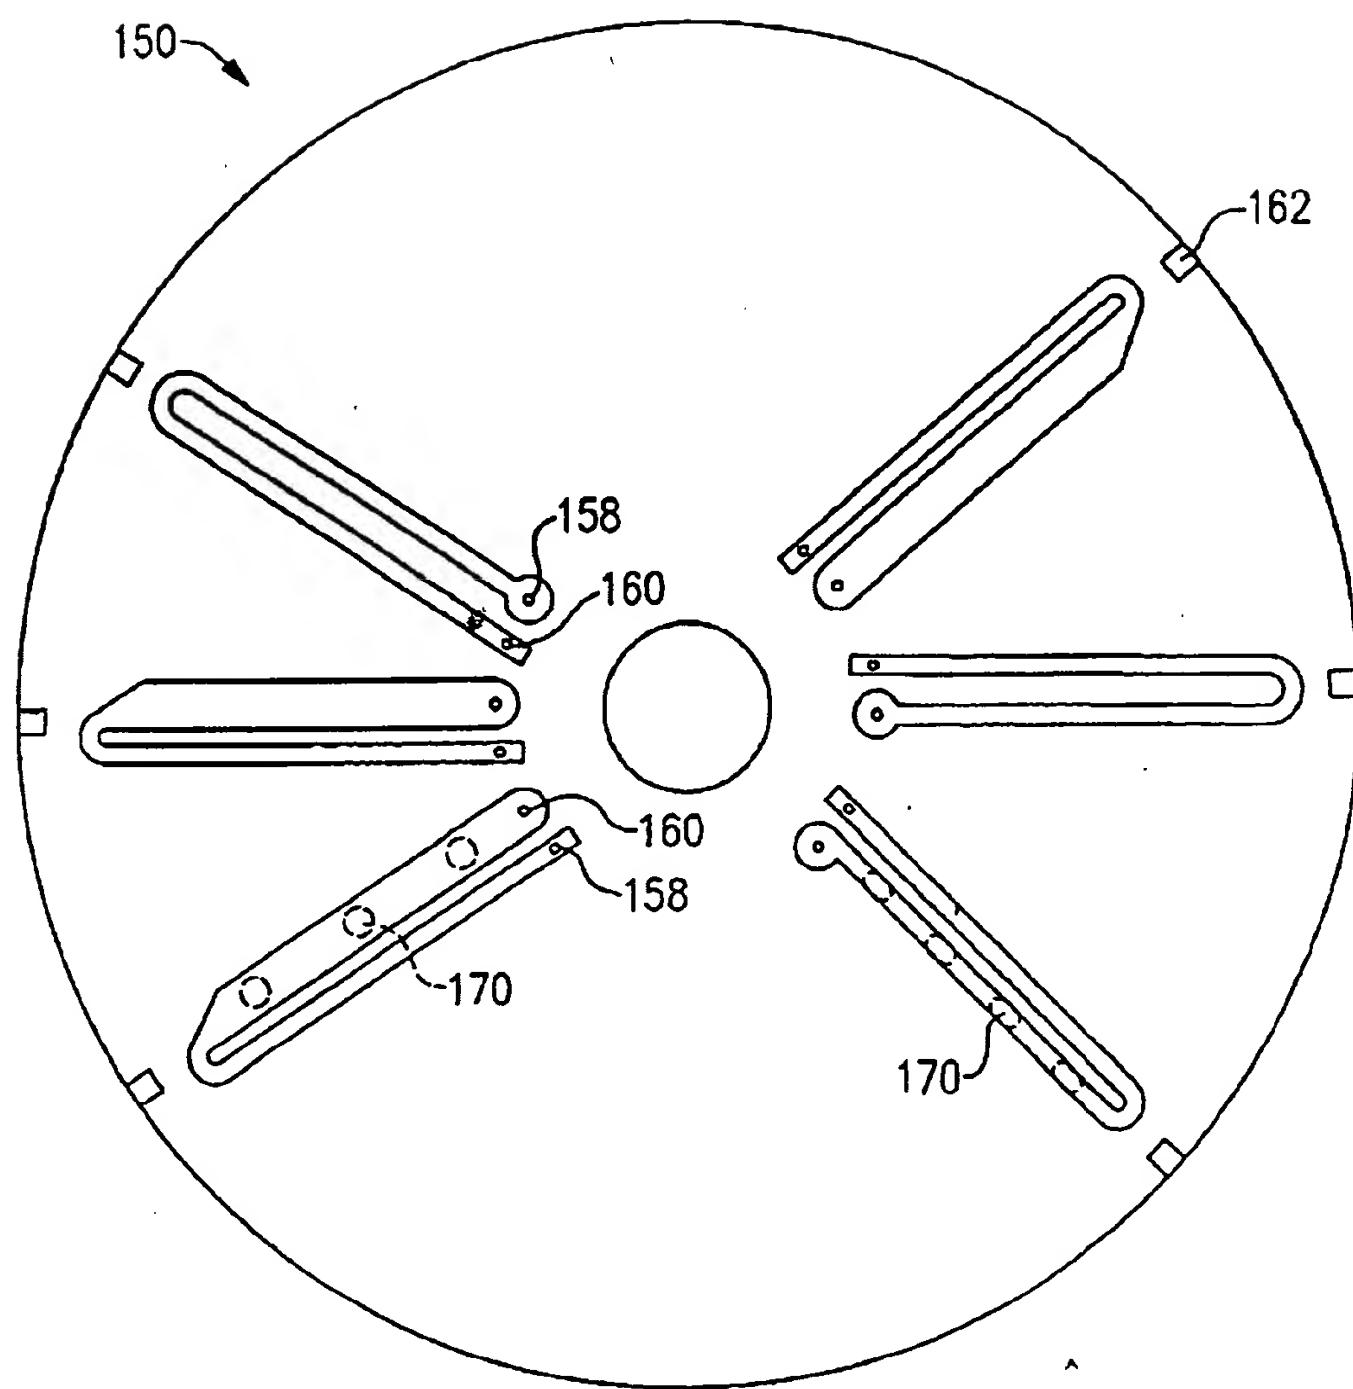


FIG.2B

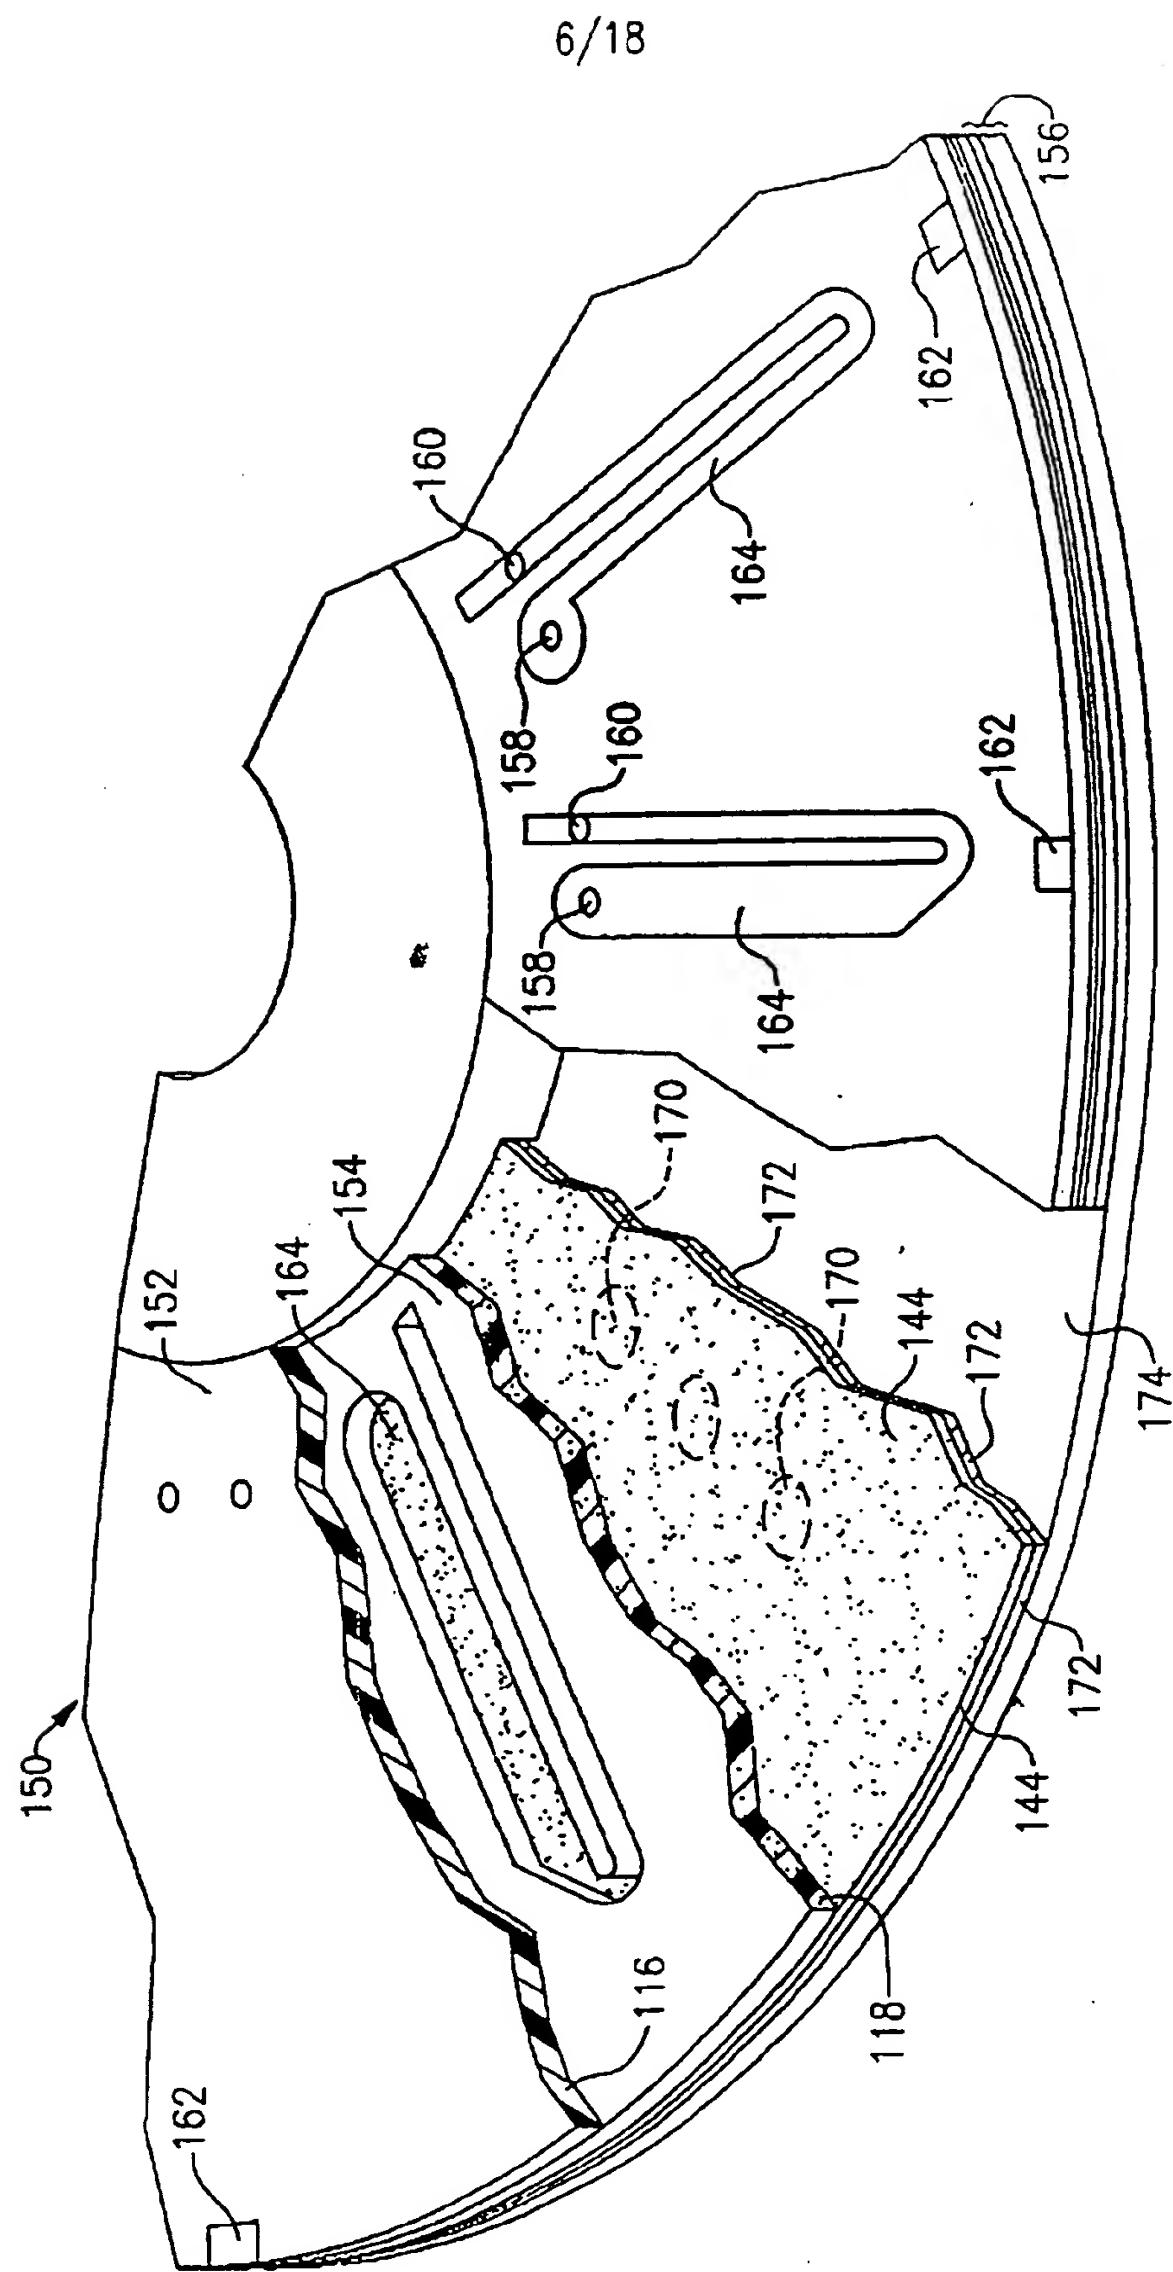


FIG. 2C

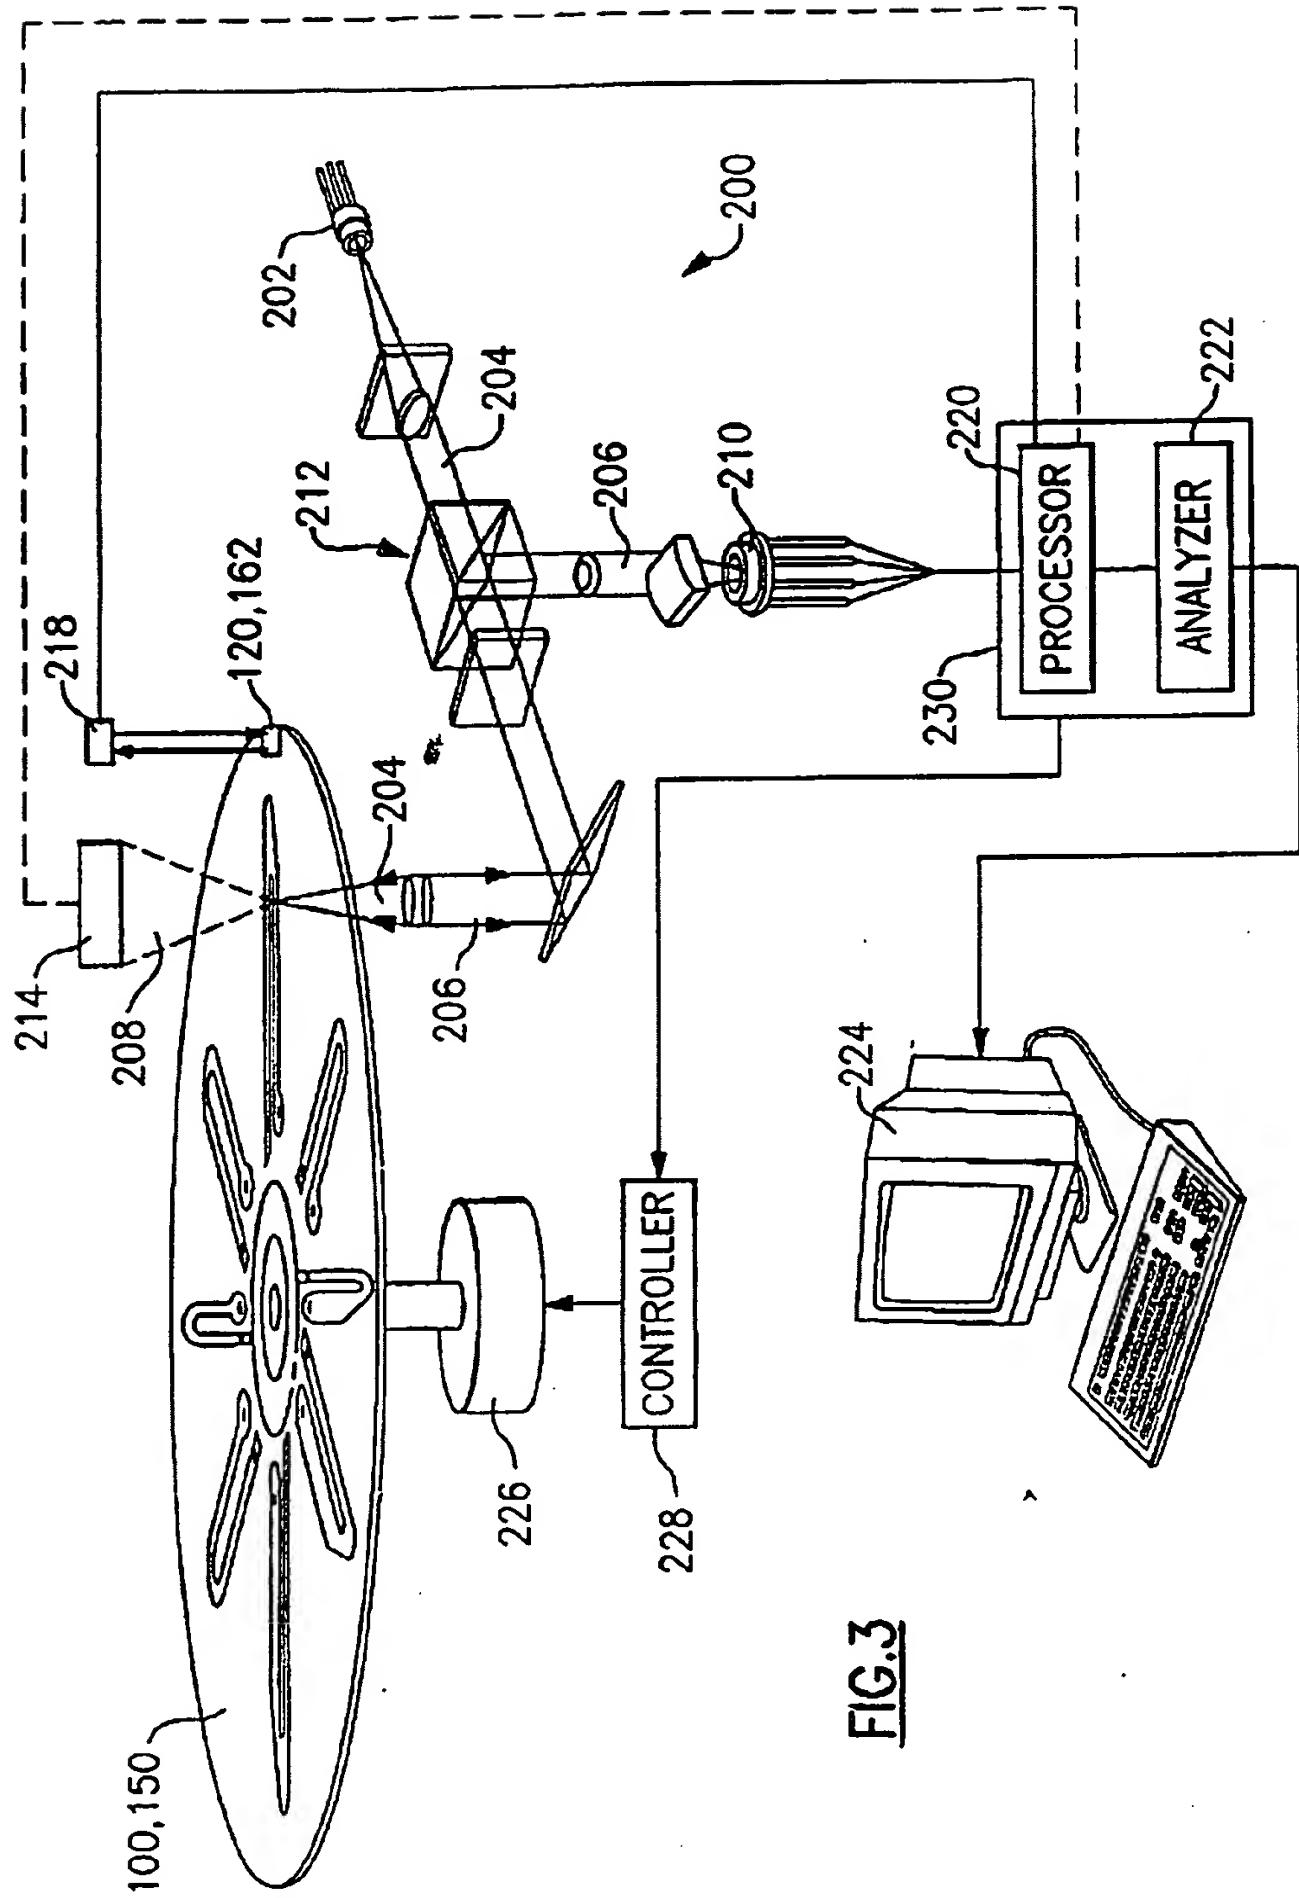


FIG.3

8/18

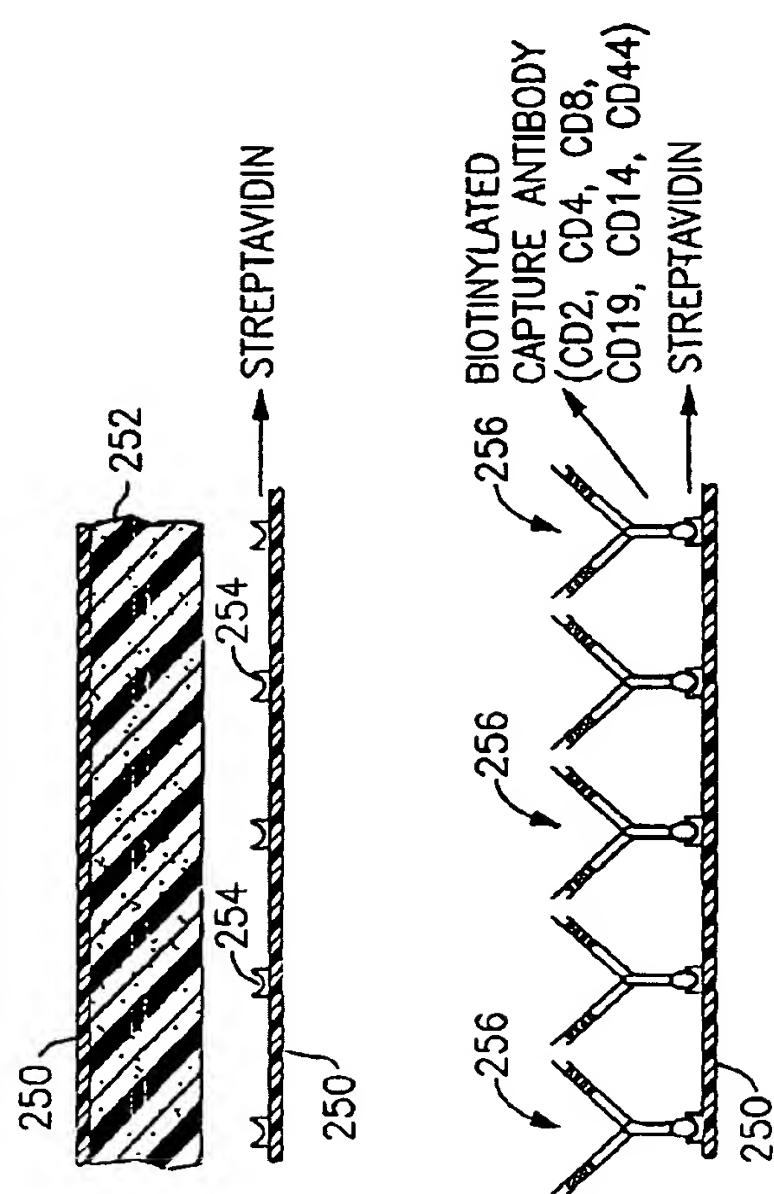
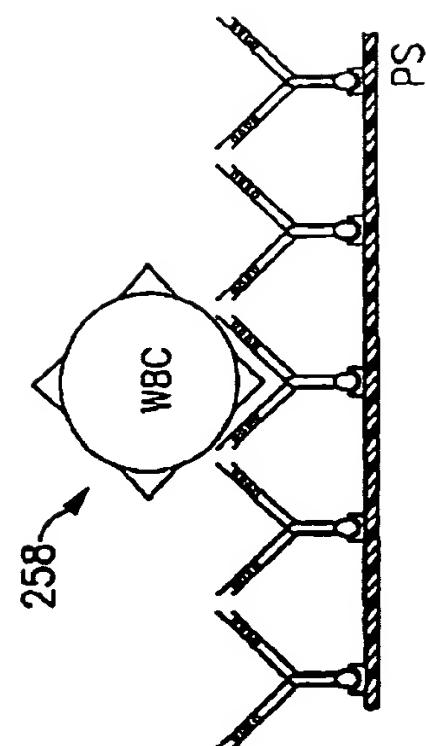
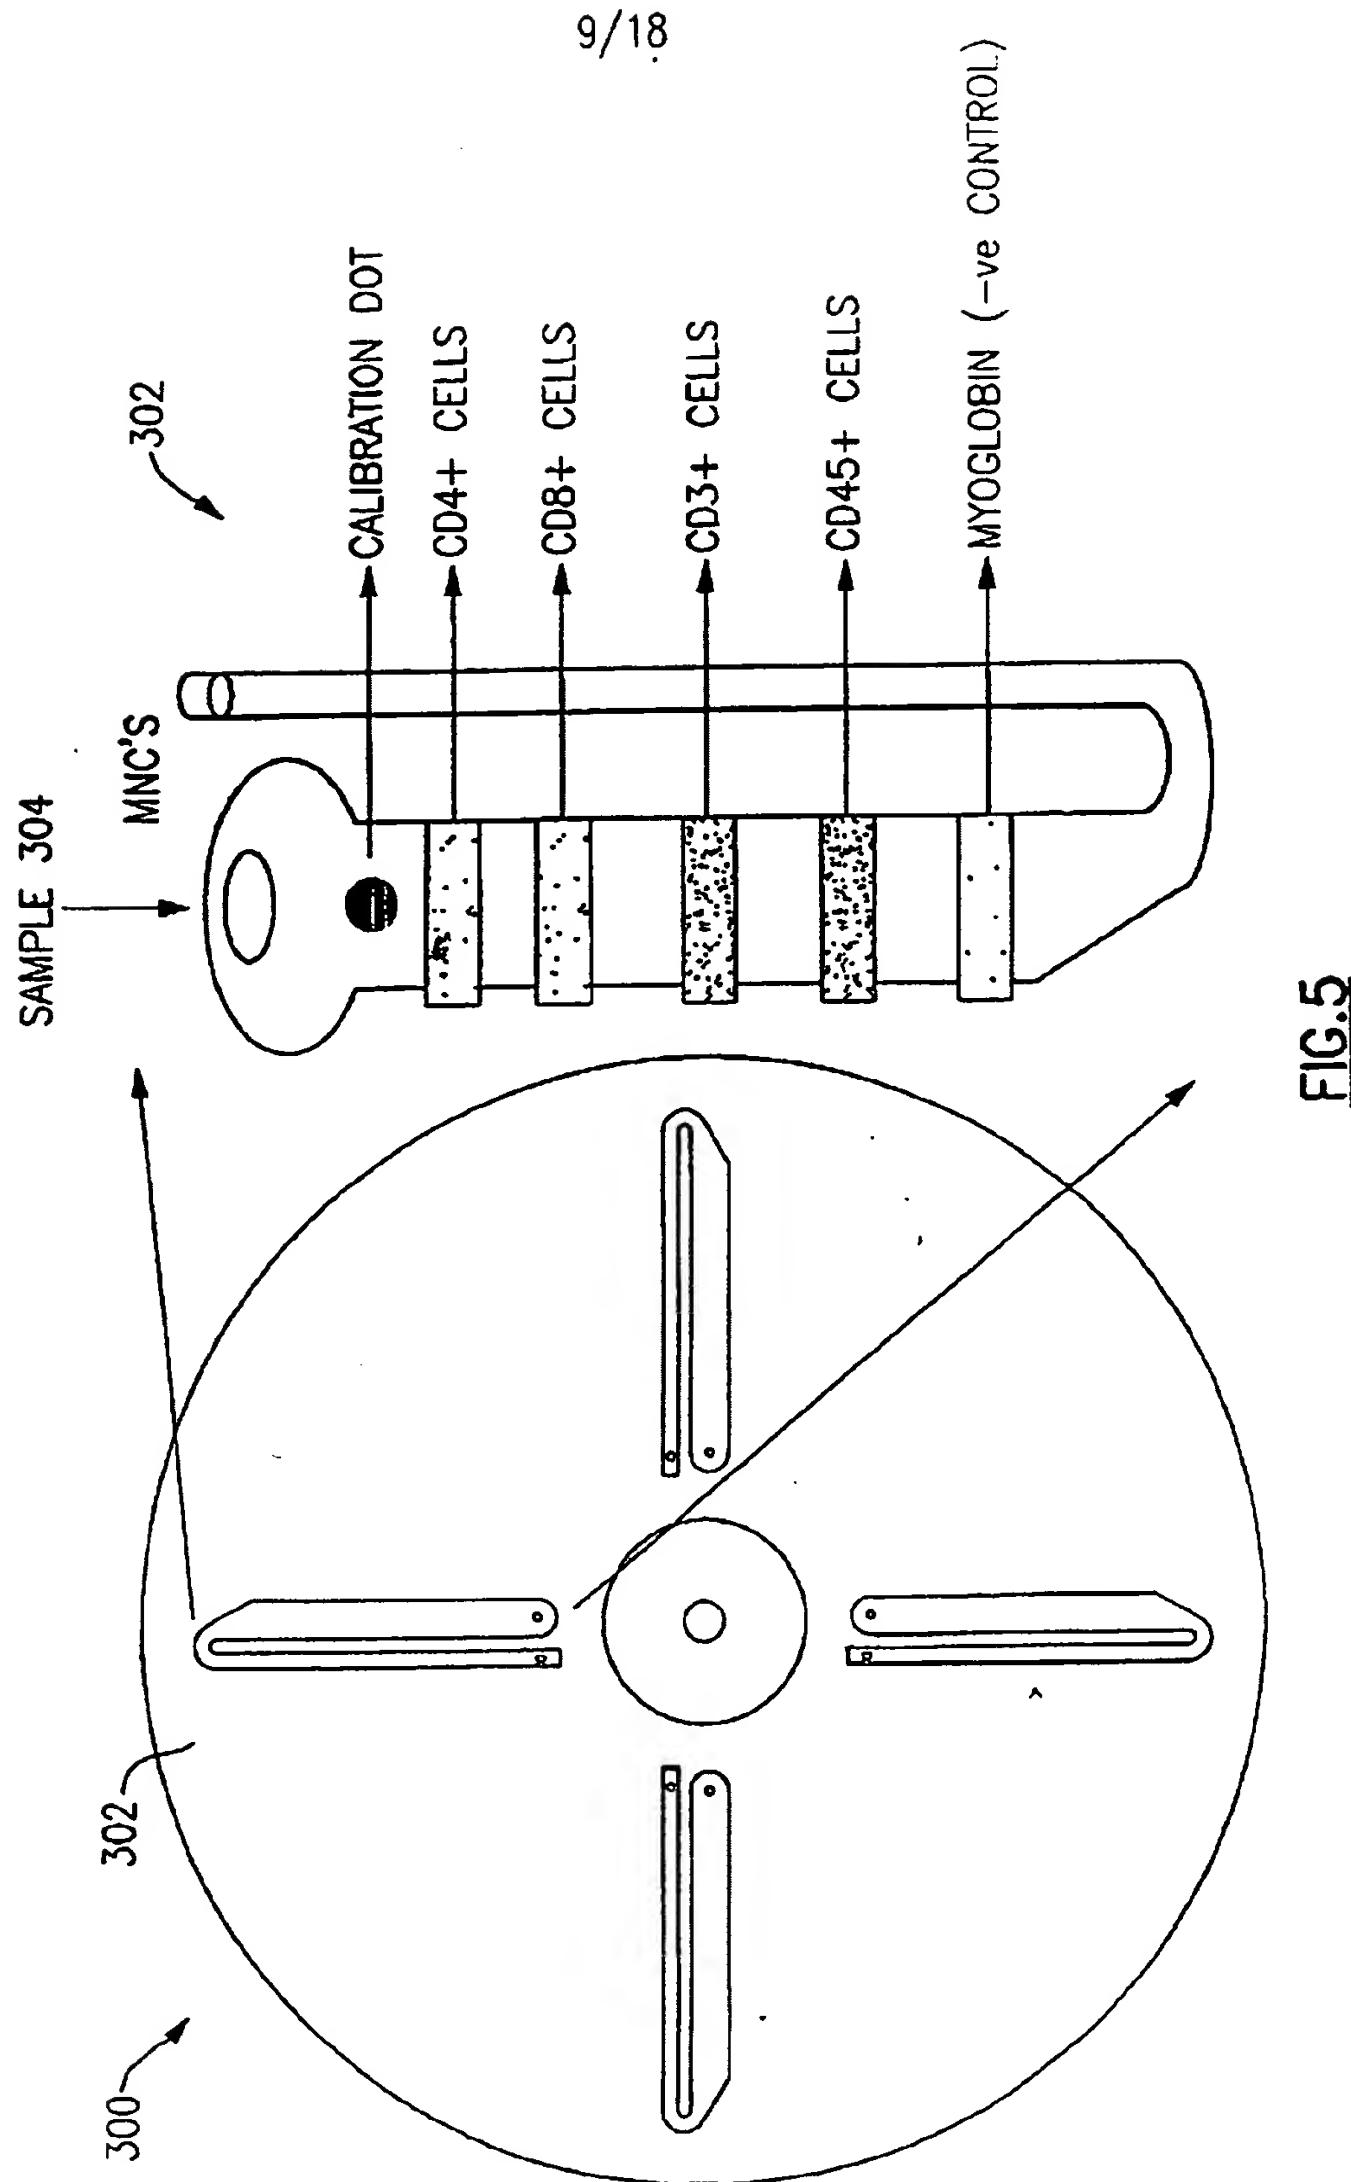
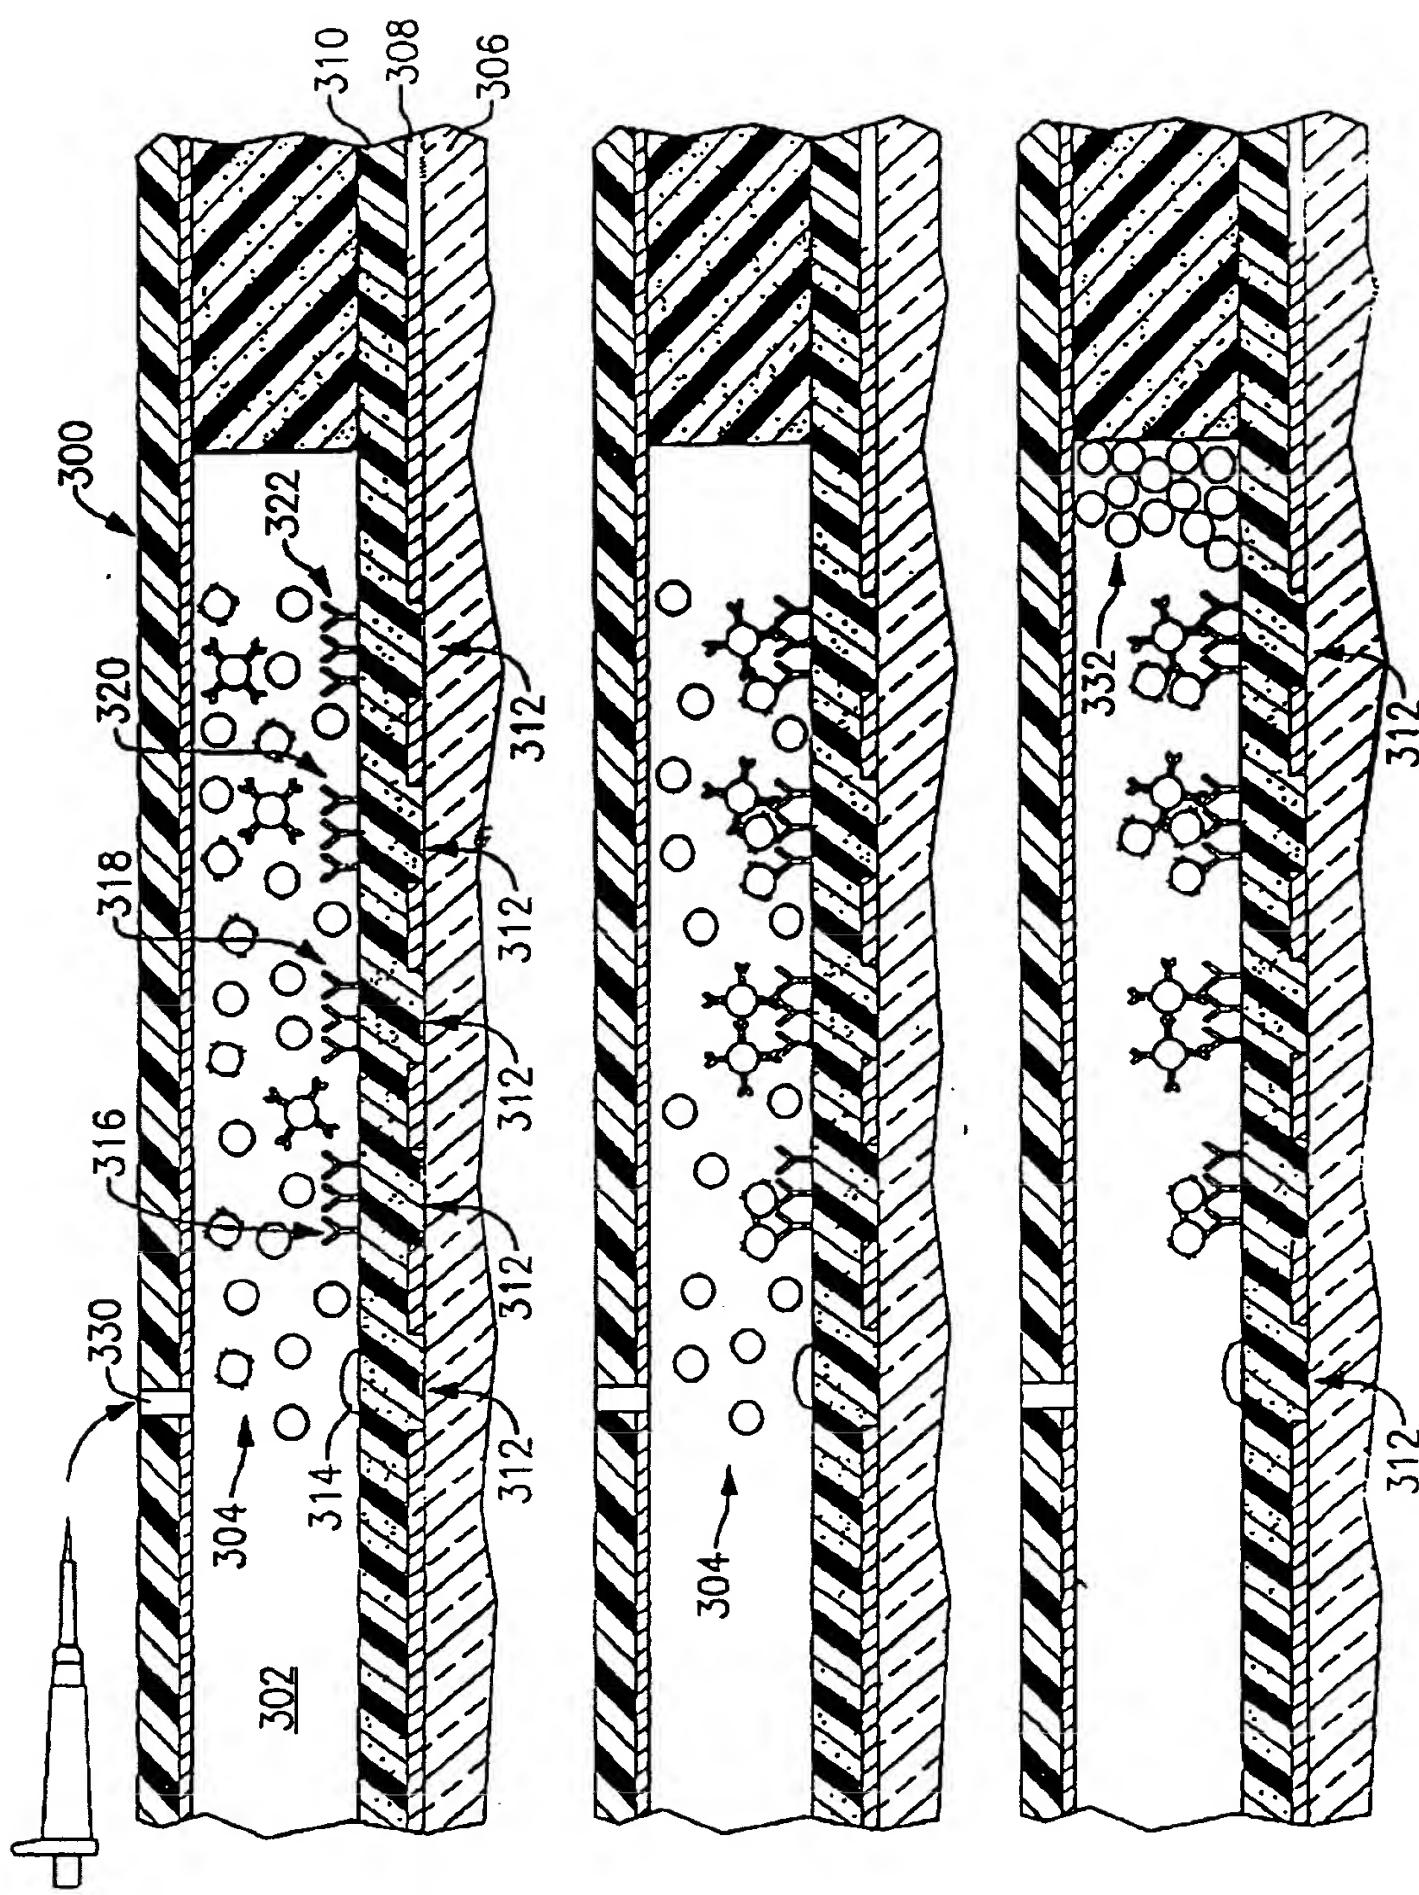


FIG. 4





**FIG. 6A**

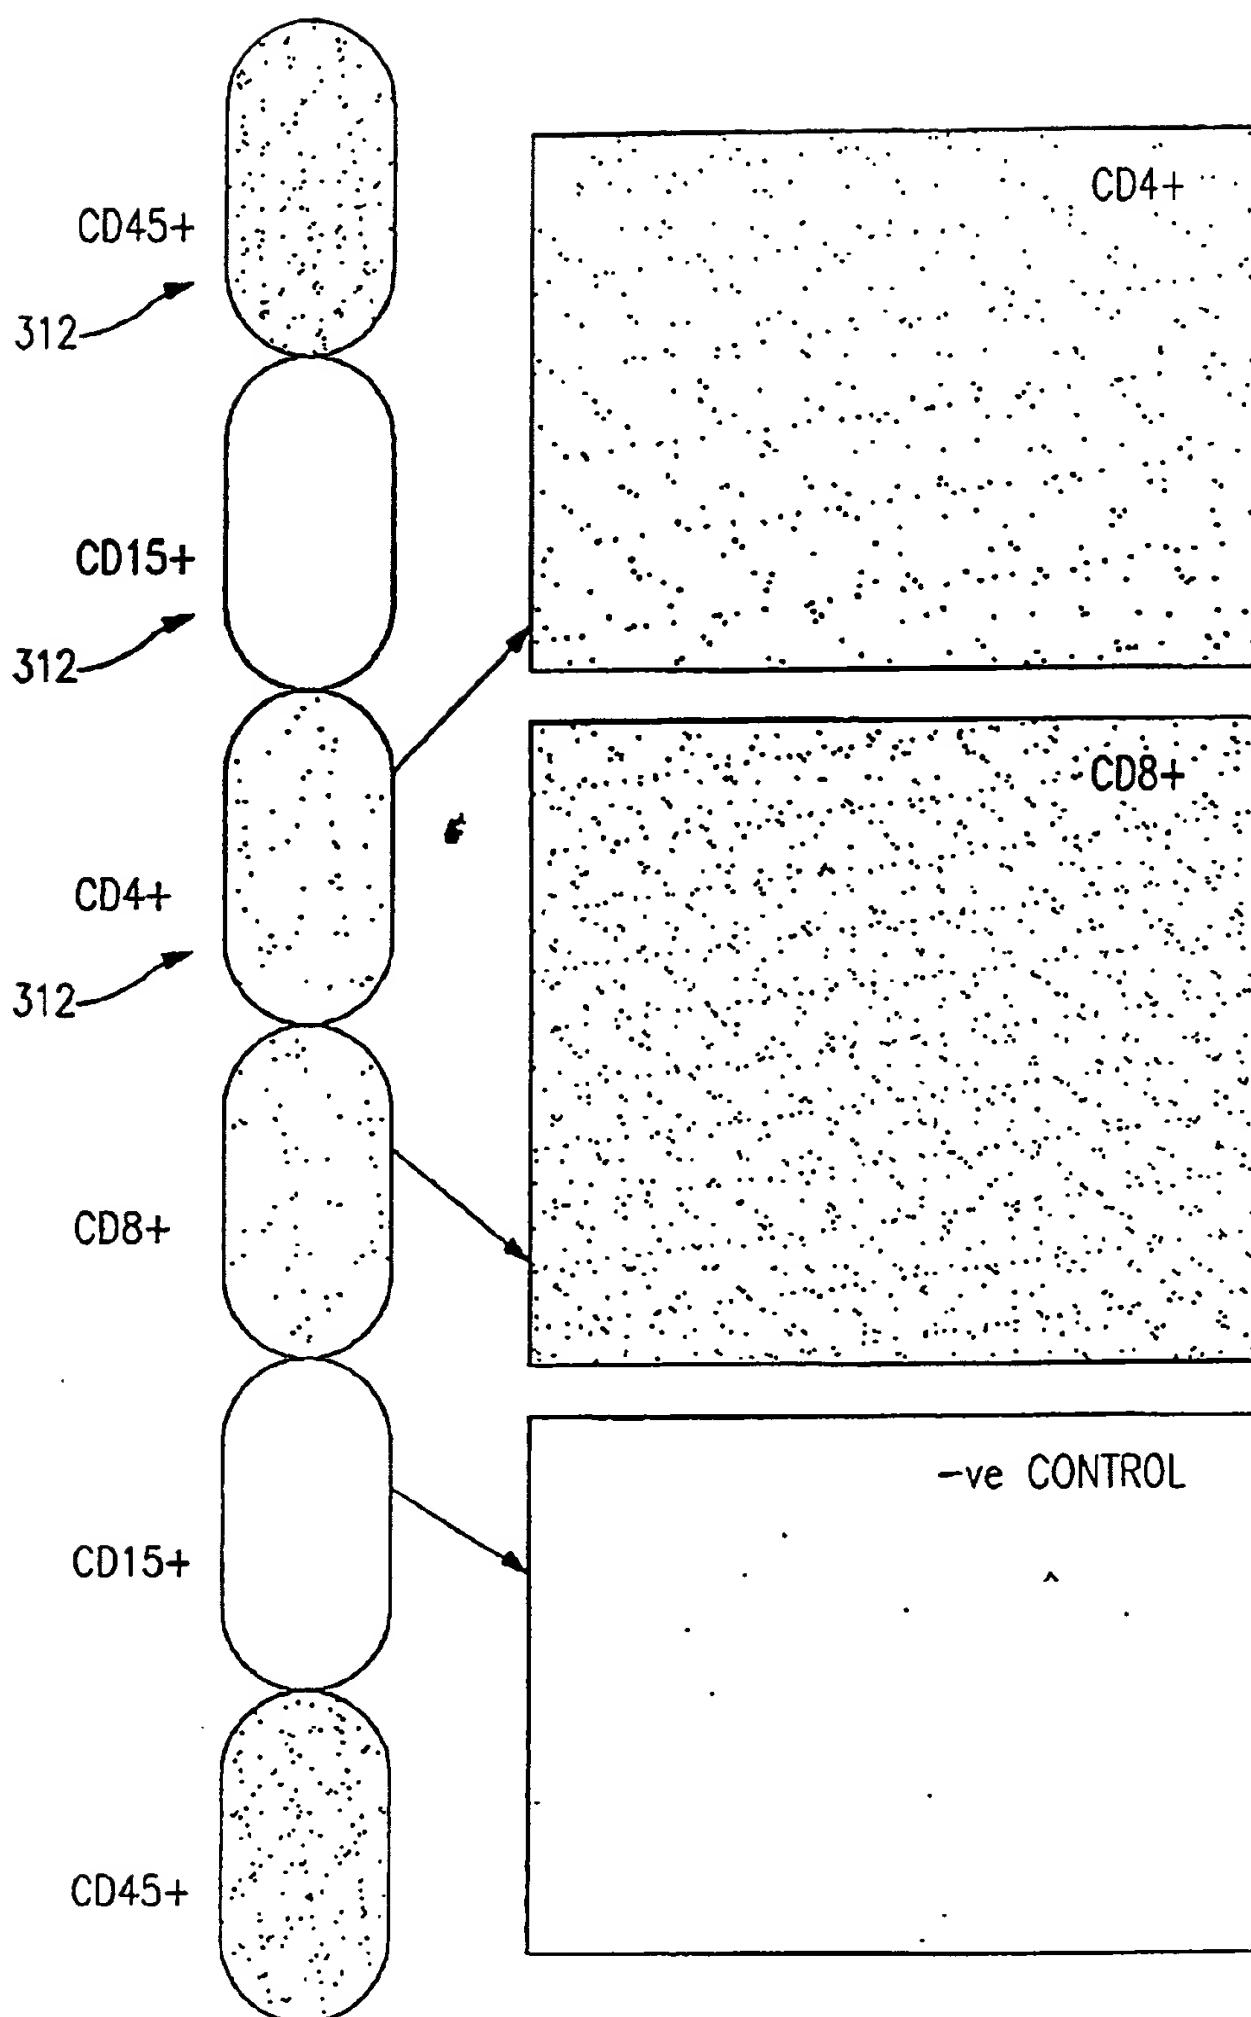


FIG.7A

12/18


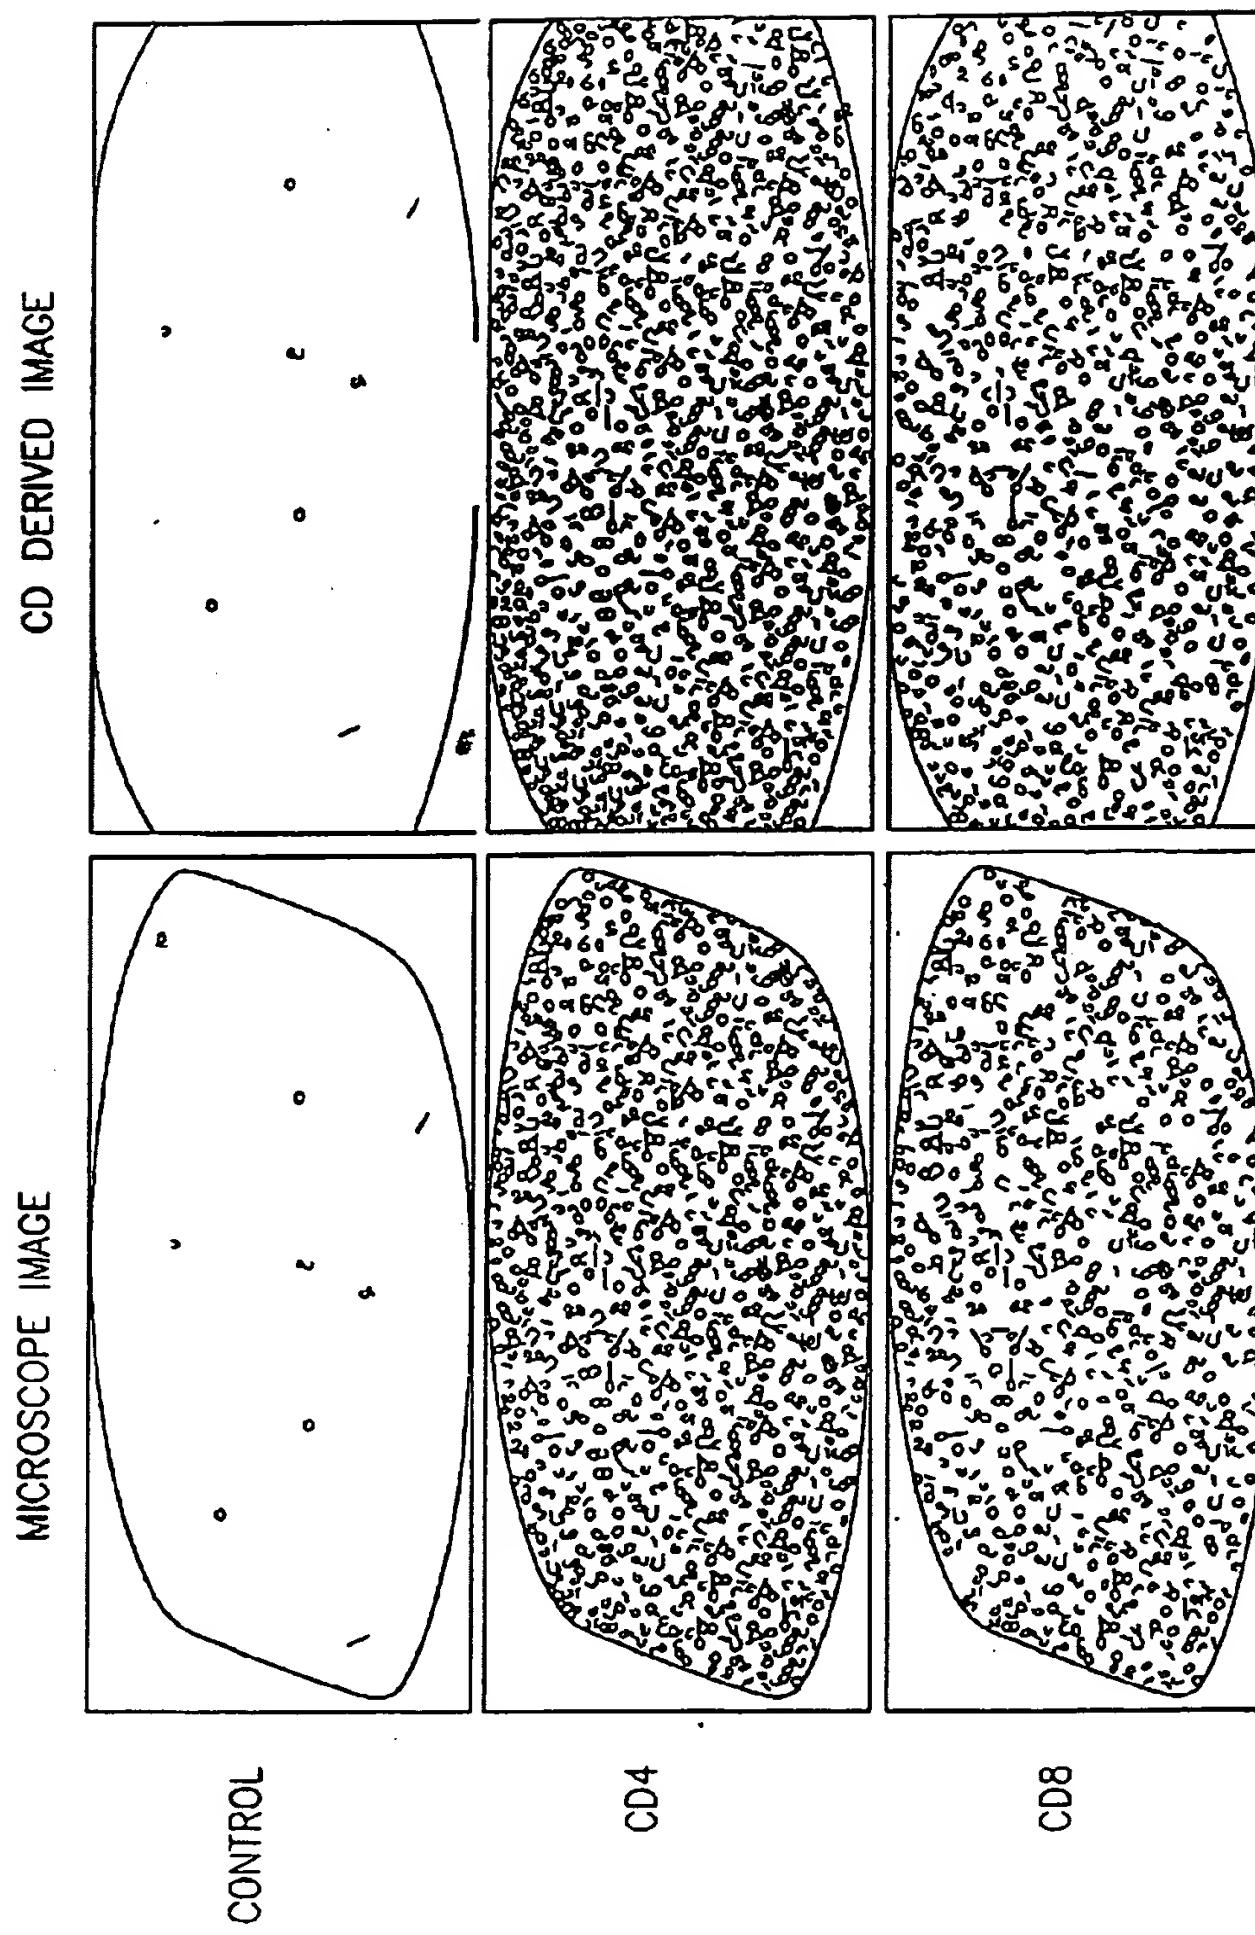


FIG. 7B

13/18

CD DERIVED IMAGE

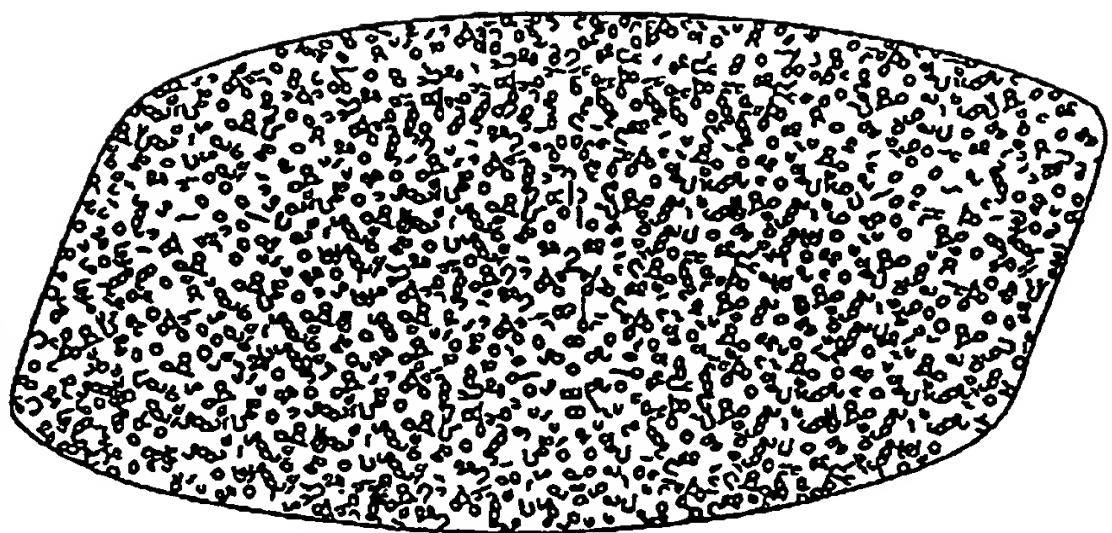

MICROSCOPE IMAGE

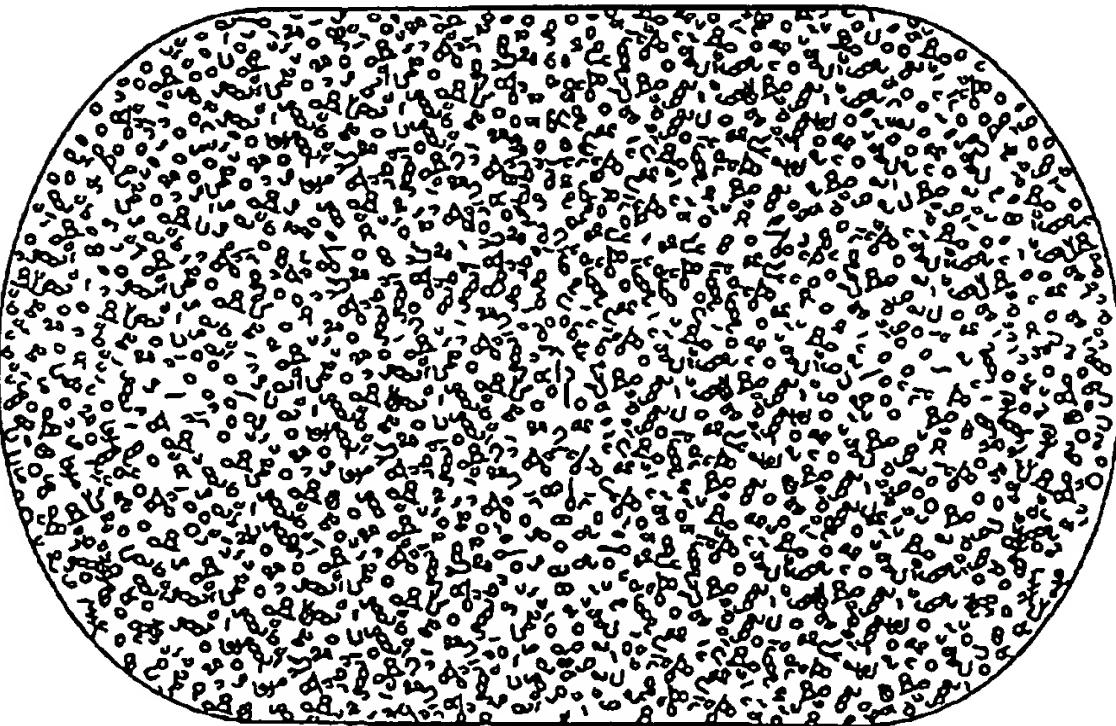


FIG.8

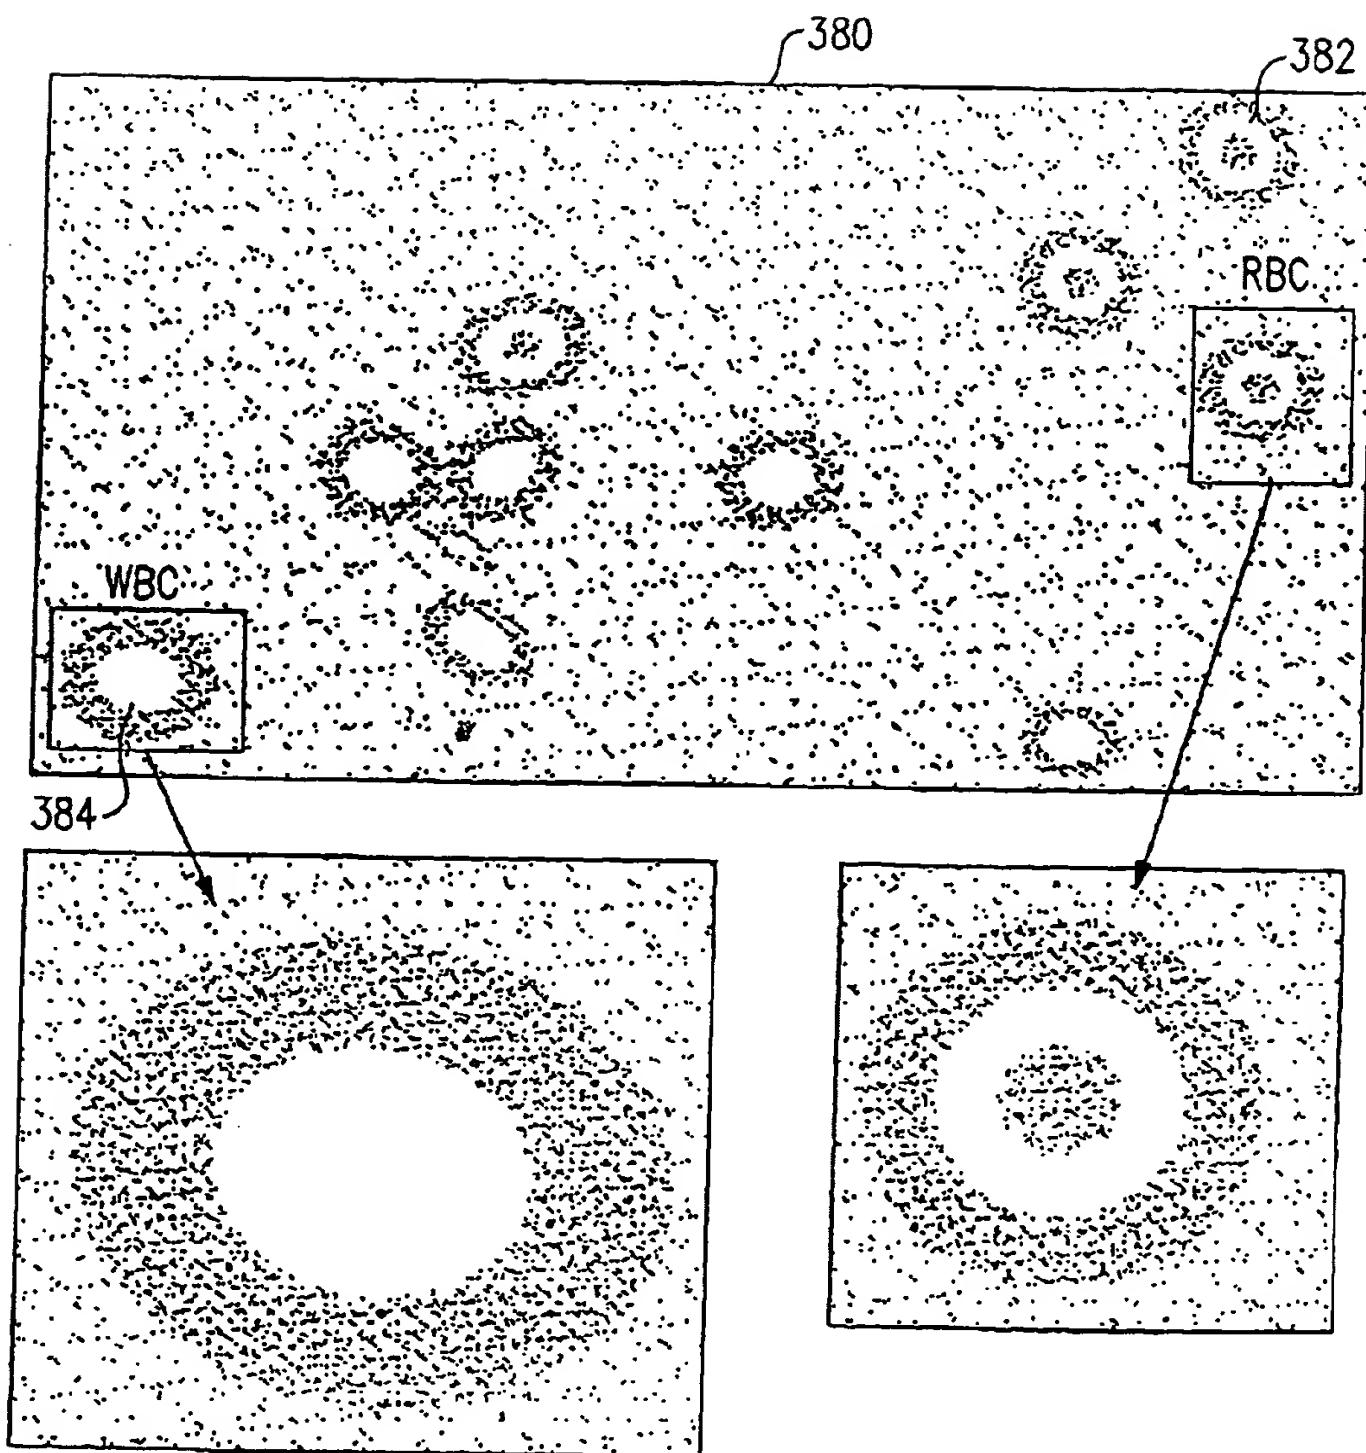


FIG.9

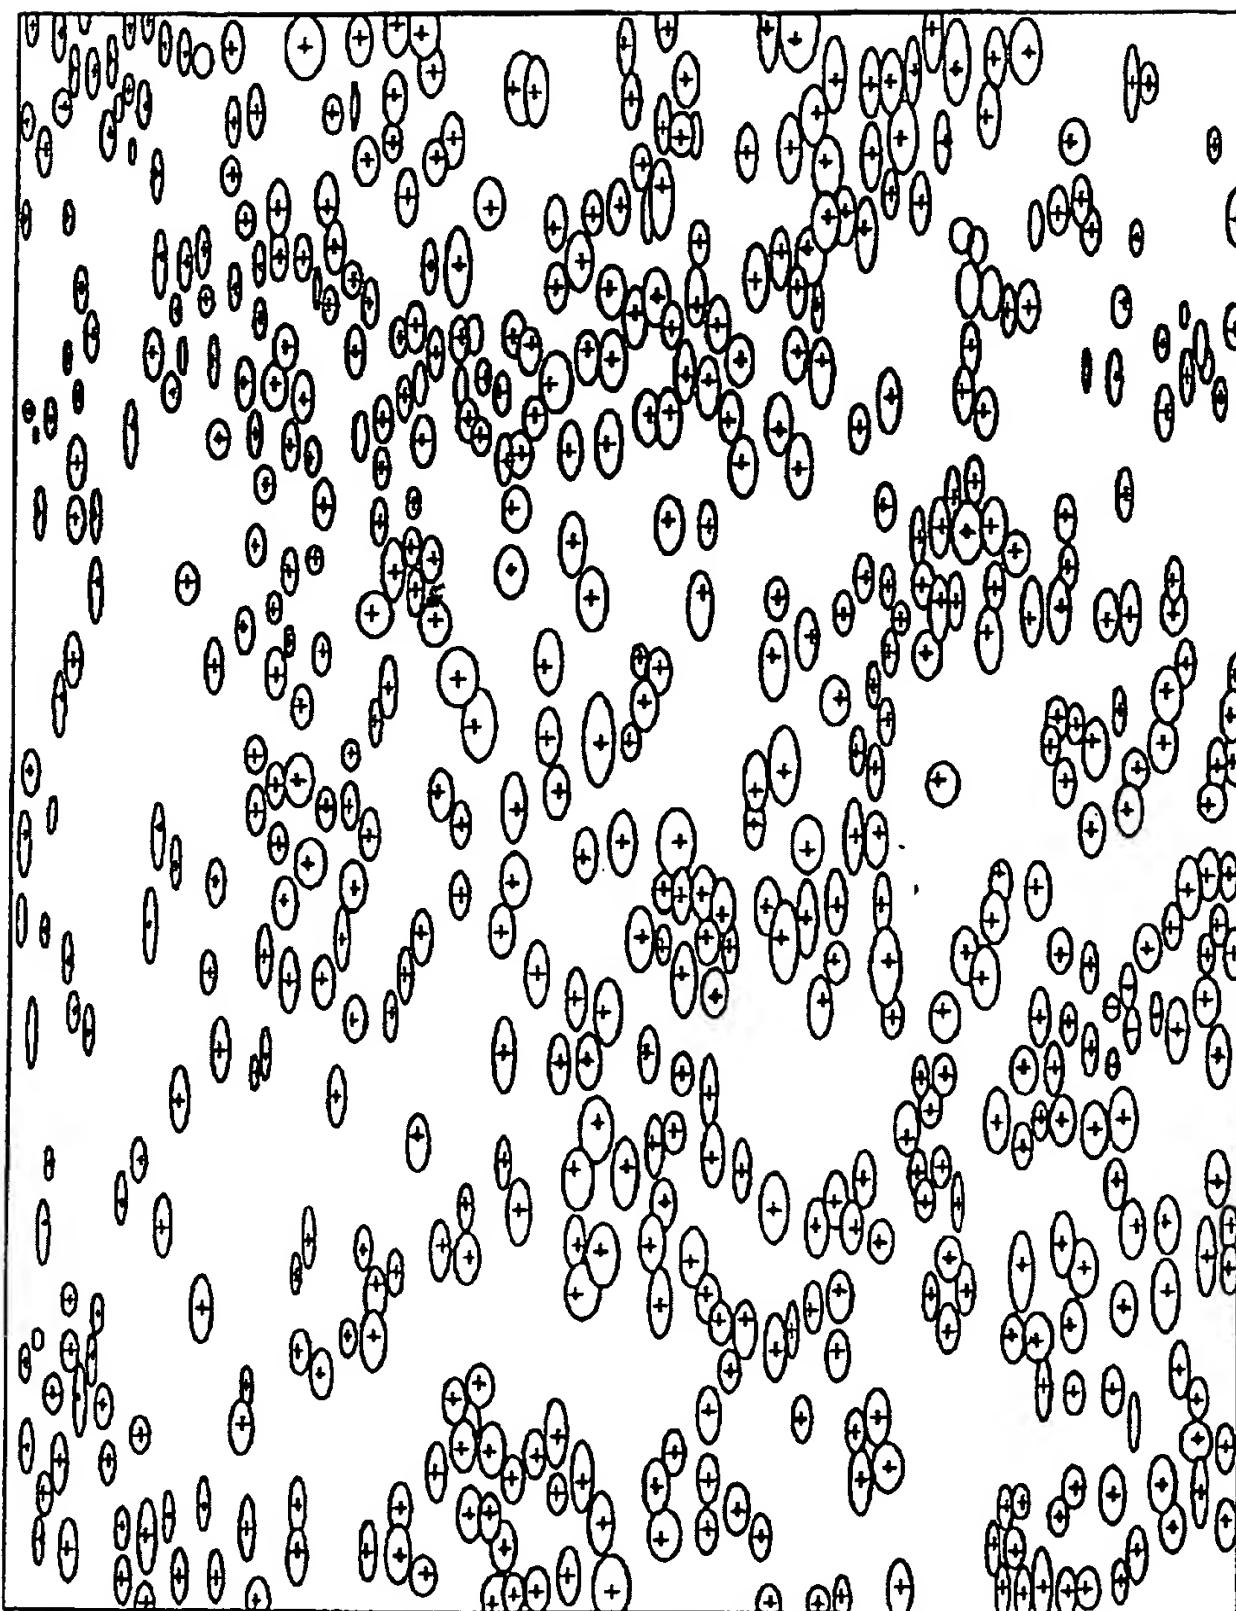


FIG. 10

16/18

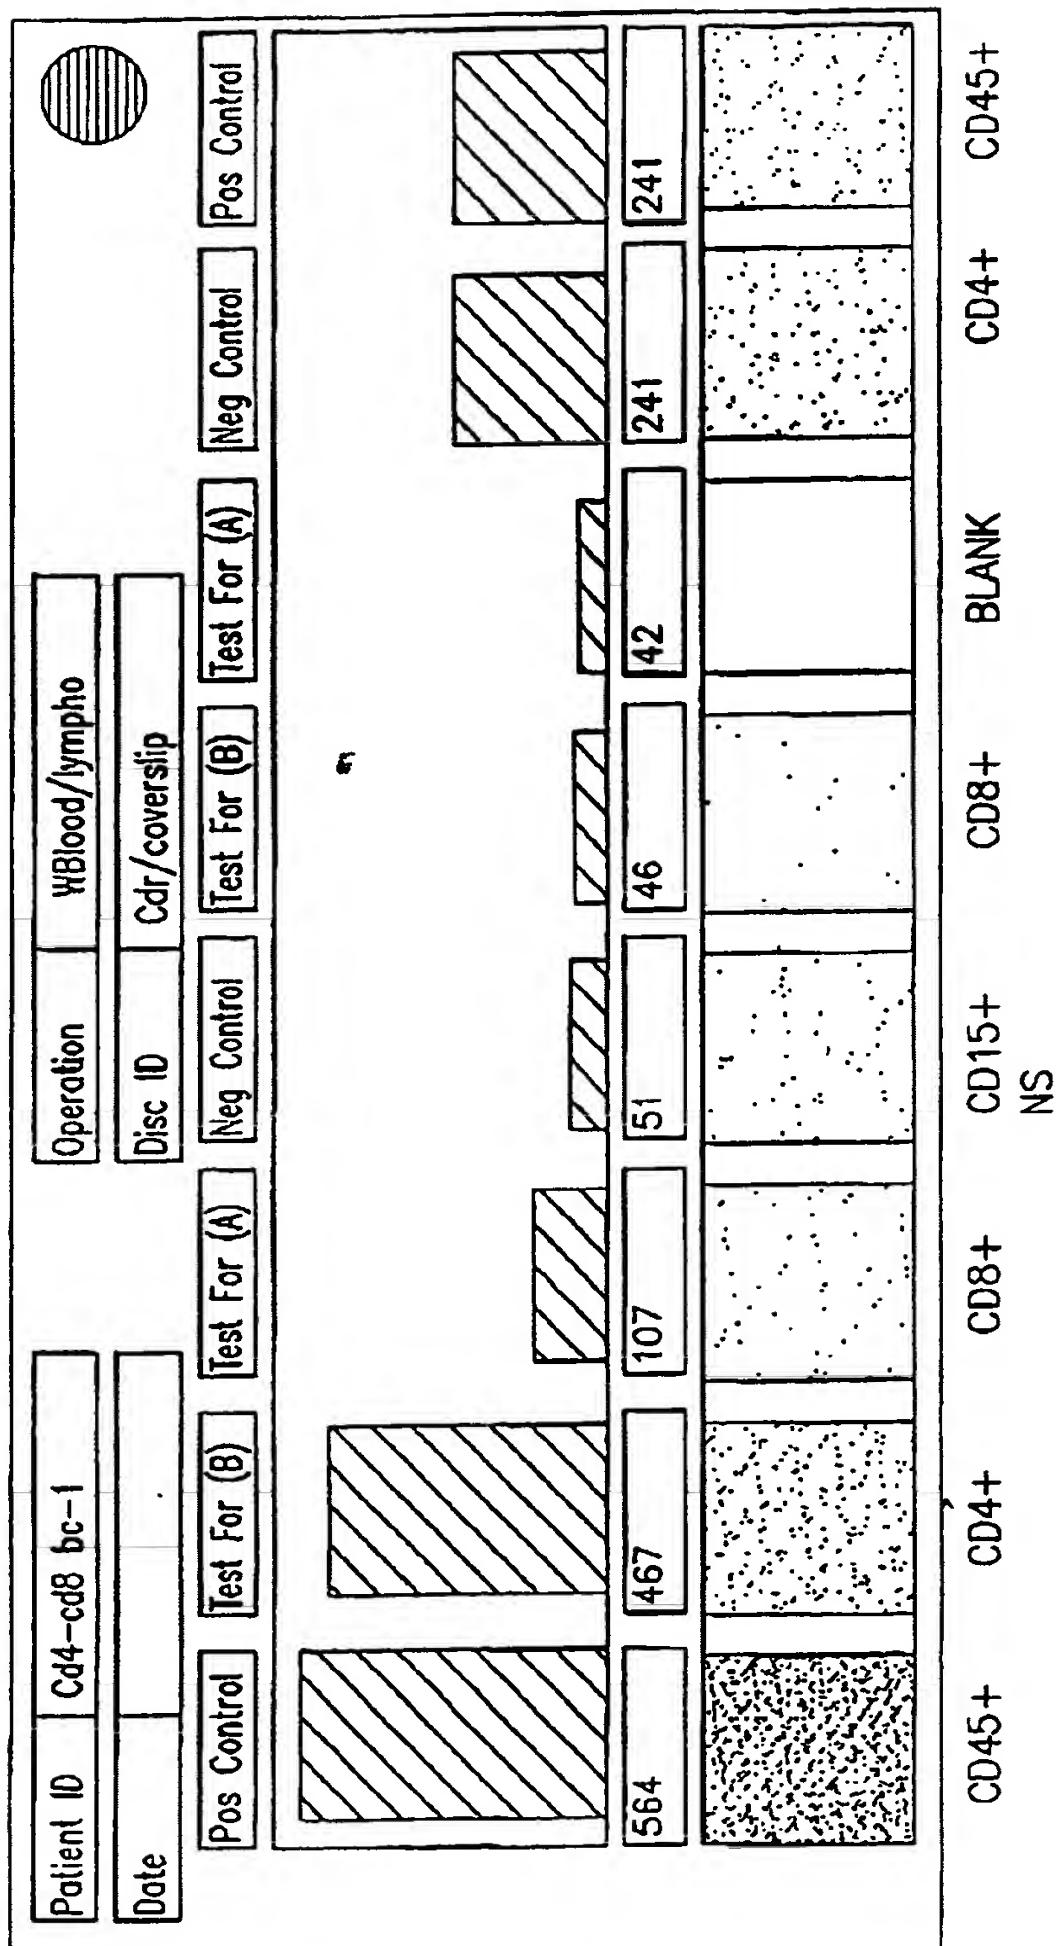


FIG. 11

